


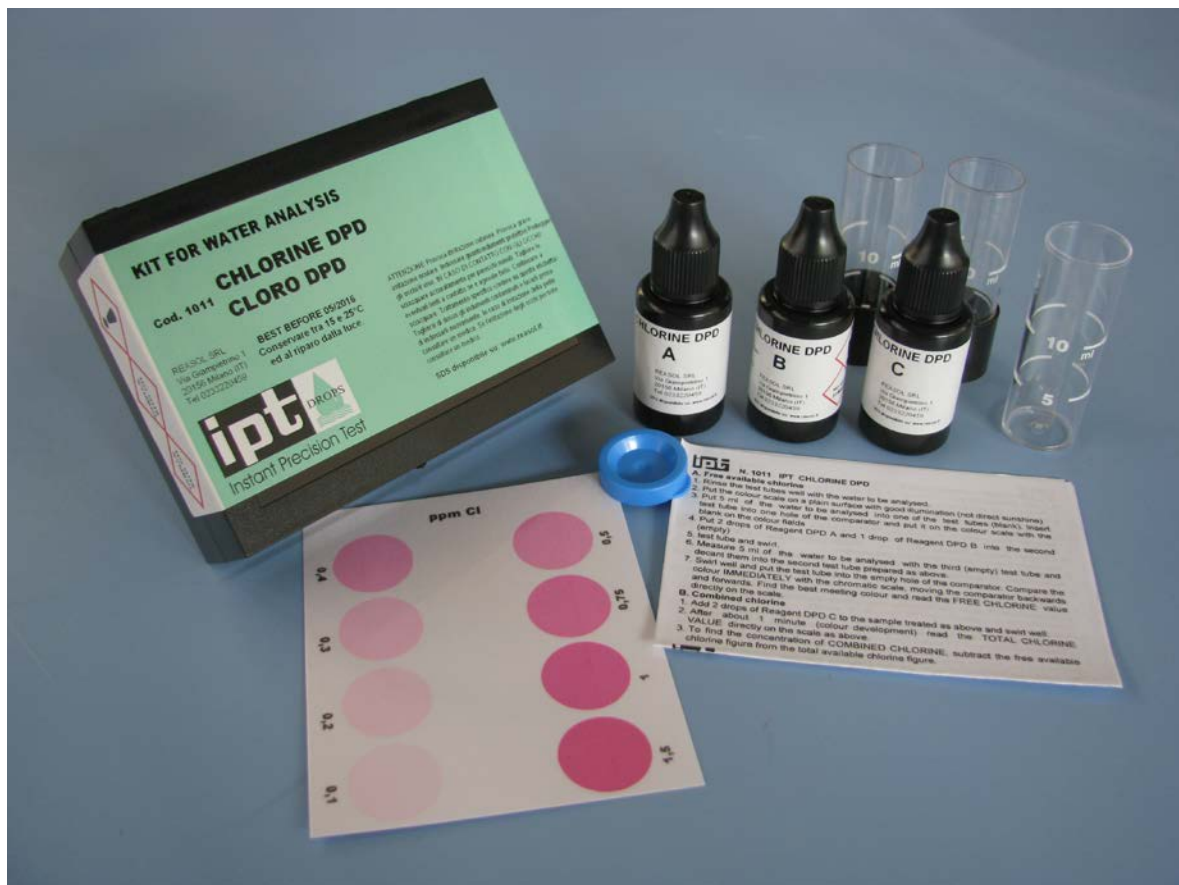

Code N° 1011 IPT CHLORINE DPD

SENSITIVITY: 0,1 ppm Cl_2

TEST QUANTITY: 150

KIT CONTAINS:

- 1 bottle 15cc reagent Chlorine DPD A
- 1 bottle 15cc reagent Chlorine DPD B
- 1 bottle 15cc reagent Chlorine DPD C
- 3 test tubes 10cc with one stopper
- 1 color scale 0,1-1,5 ppm
- comparator
- use directions

NOTES:

- This kit measures the free chlorine and the total chlorine. The difference is given by the combined chlorine.
- For higher precision we recommend the HYDROCHECK COLORTTEST (color comparison), HYDROCHECK MONOTEST or SPECTRATEST (both for use with a spectrophotometer).

SPARE PARTS:

- reagent Chlorine DPD A, 6 bottles 15cc
- reagent Chlorine DPD B, 6 bottles 15cc
- reagent Chlorine DPD C, 6 bottles 15cc
- test tube 10cc, 12
- 1 color scale 0,1-1,5 ppm

Code N° 3239

Code N° 3240

Code N° 3241

Code N° 3312

Code N° 3404