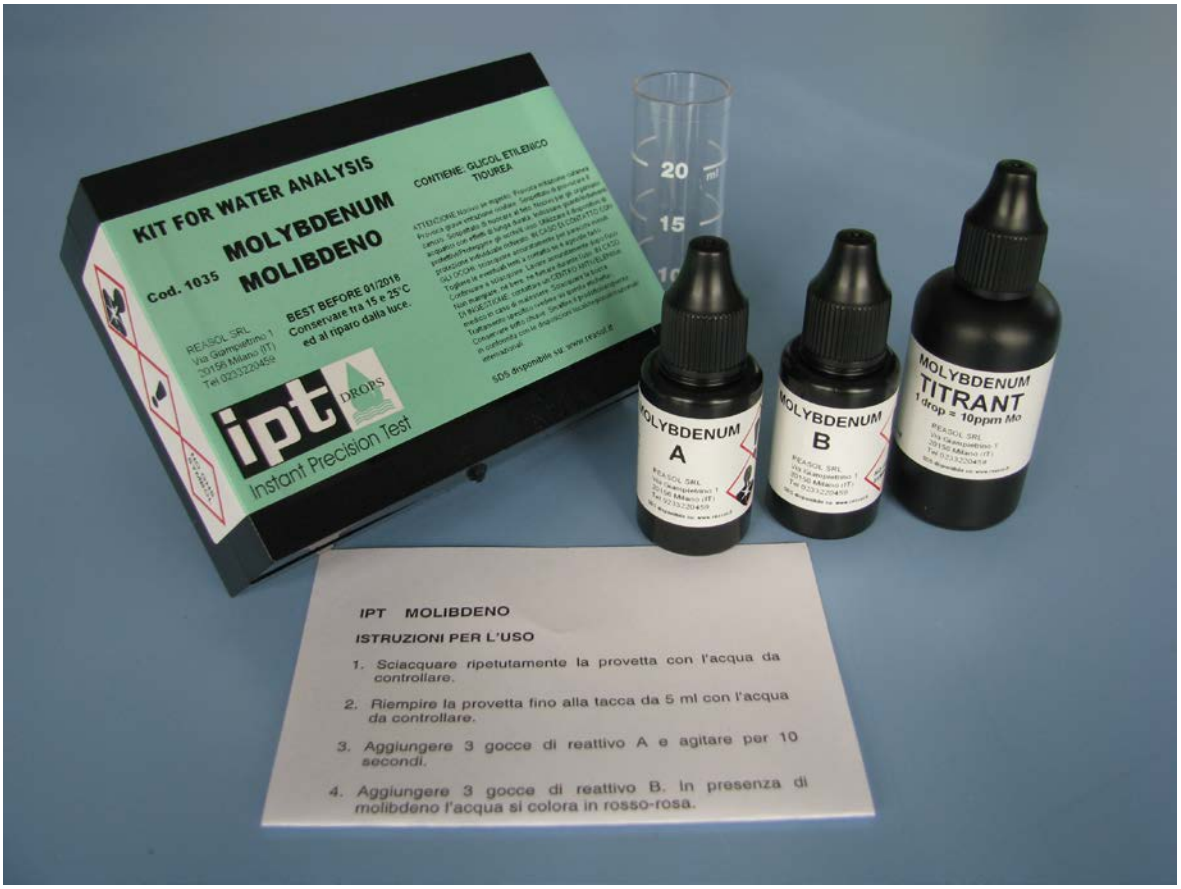

Code N° 1035

IPT MOLYBDAENUM

SENSITIVITY: 10 ppm Mo

TEST QUANTITY: 6.000 ppm Mo

KIT CONTAINS:

- 1 bottle 25cc titrant Molybdaenum
- 1 bottle 15cc indicator Molybdaenum
- 1 bottle 15cc reagent A Molybdaenum
- 1 test tube 20cc
- use directions

NOTES:

- The titrant has a limited stability and musyt be stored in the dark, in the well closed bottle, between 10 and 15 degrees C.
- For higher precision we recommend the HYDROCHECK kits.

SPARE PARTS:

• titrant, 6 bottles 25cc	Code N° 3123
• titrant, 6 bottles 250cc	Code N° 3124
• indicator, 6 bottles 15cc	Code N° 3263
• reagent A, 6 bottles 15cc	Code N° 3265
• test tube 20cc, 10	Code N° 3310