


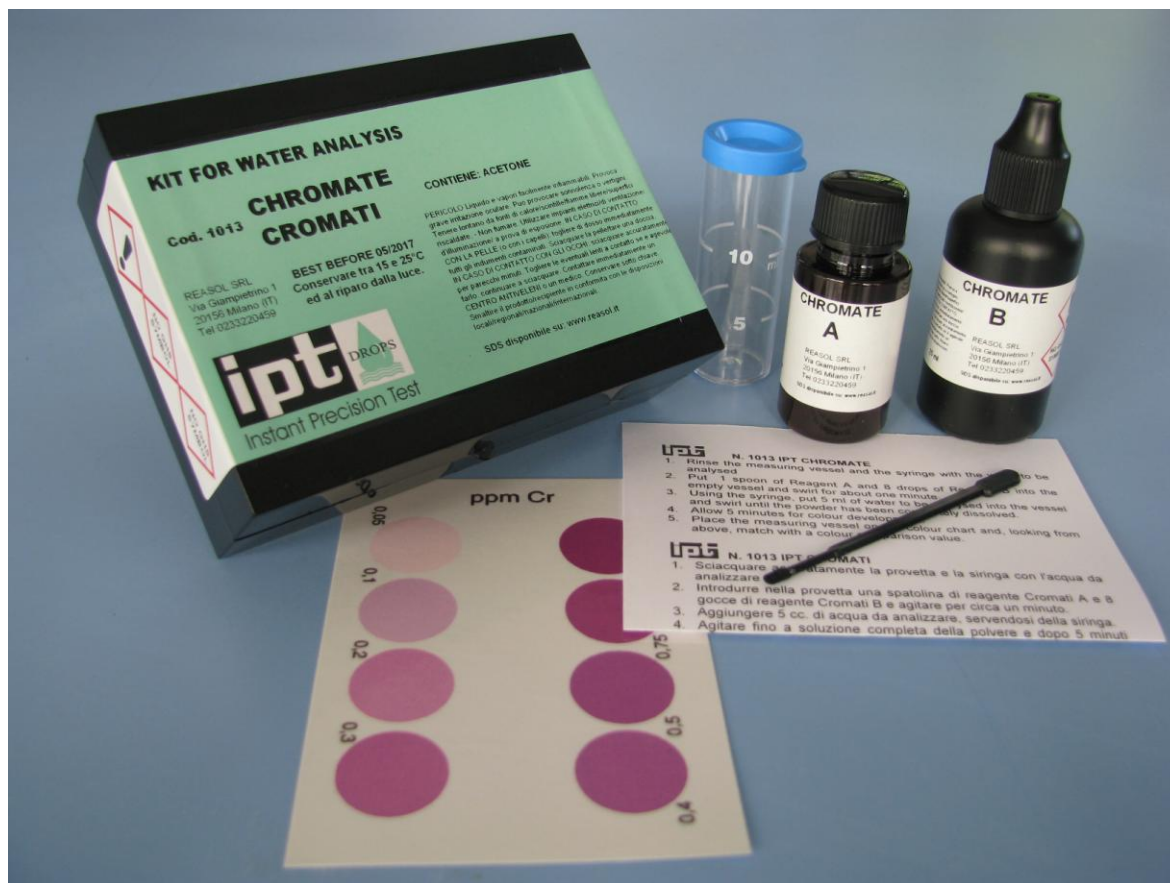

Code N° 1013 IPT CHROMATE

SENSITIVITY: 0,05 ppm Cr

RANGE: 0,05 - 0,1 - 0,2 - 0,3 - 0,4 - 0,5 - 0,75 - 1,0 ppm Cr

TEST QUANTITY: 50

KIT CONTAINS:

- 1 bottle 25ml reagent Chromate A
- 1 bottle powder reagent Chromate B
- 1 test tube 10ml with stopper
- 1 color scale
- 1 spatula
- use directions

NOTES:

The method measures the Cr^{+6} .

For higher precision we recommend the HYDROCHECK COLORTTEST (color comparison), HYDROCHECK MONOTEST or SPECTRATEST (both for use with a spectrophotometer).

SPARE PARTS:

- reagent A, 6 bottles 25ml
- reagent B, 6 bottles
- 12 test tube 10ml,
- 1 color scale

Code N° 3209

Code N° 3210

Code N° 3312

Code N° 3406

INTERFERENCE

Nitrates > 1 ppm.

Calcium, Iron and Lead > 10 ppm.

Mercury and Molybdenum > 200 ppm.

The other substances normally present in the water do not interfere.